



Application No. 10/565,830

Applicant: Isao Karube et al.

Title: BIOSENSOR AND METHOD OF PRODUCING THE SAME

Responsive to Official Communication dated: Concurrently

REPLACEMENT SHEET

Confirmation No. Unknown

Attorney Docket No. P29193

1 / 32

FIG. 1


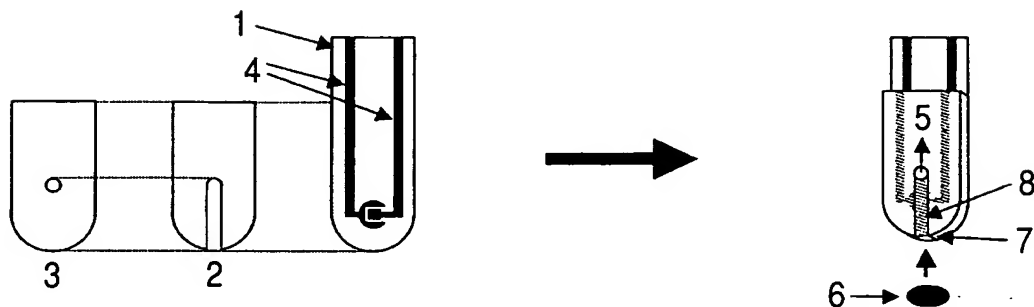


FIG. 2

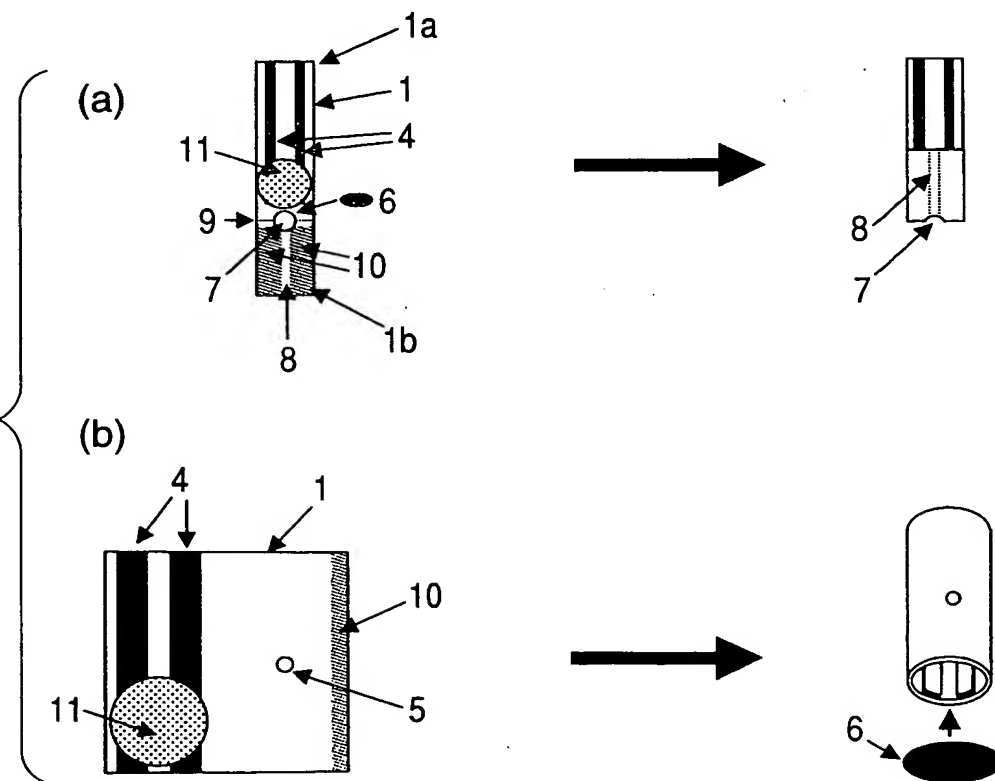

2 / 32

FIG. 3

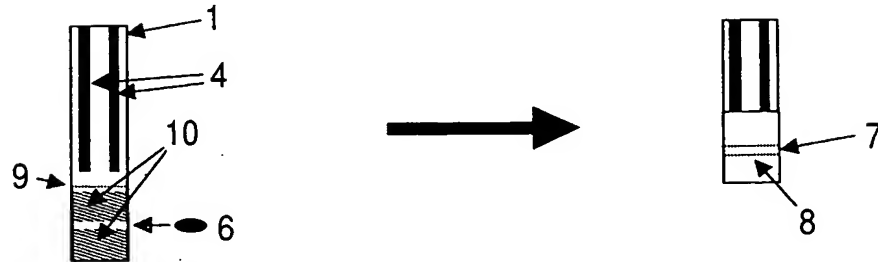


FIG. 4



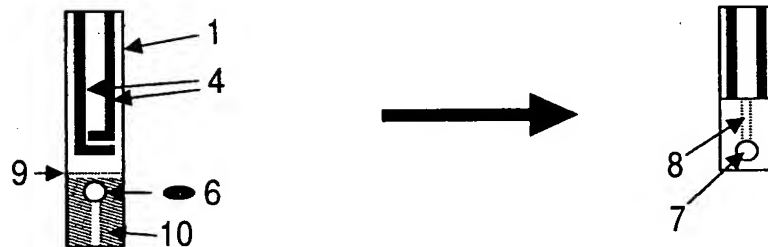



FIG. 5

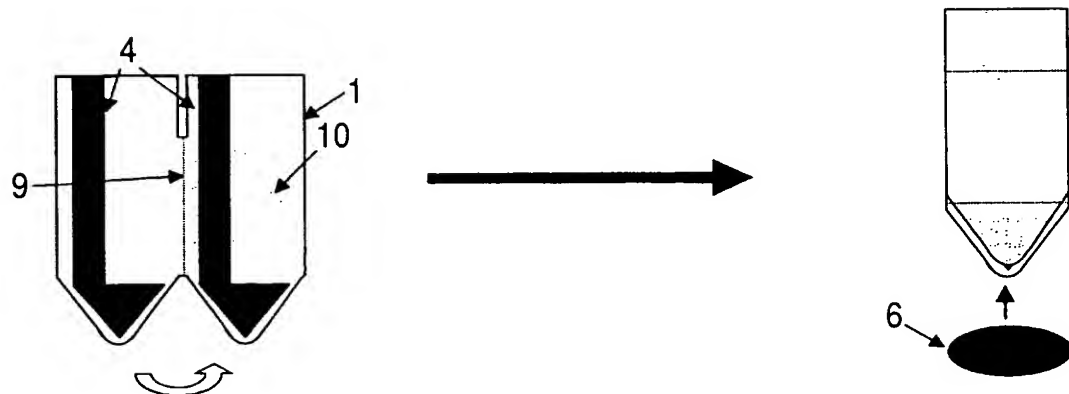


*FIG. 6*

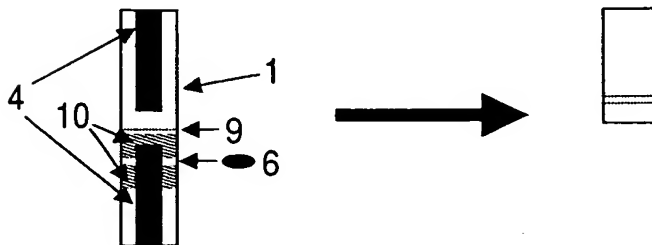


*FIG. 7*

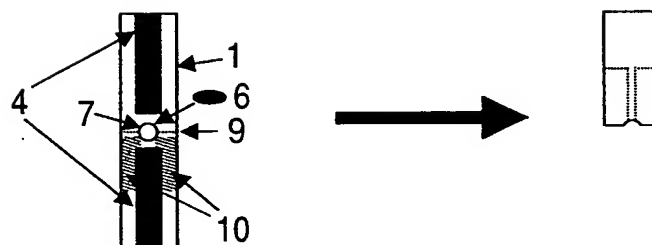

*FIG. 8*

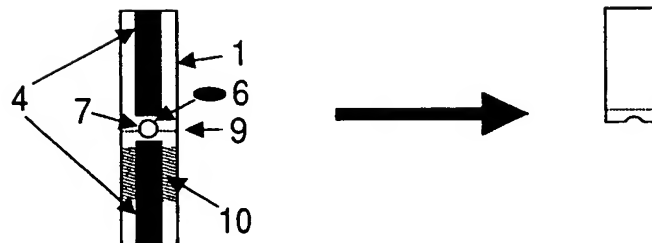

*FIG. 9*

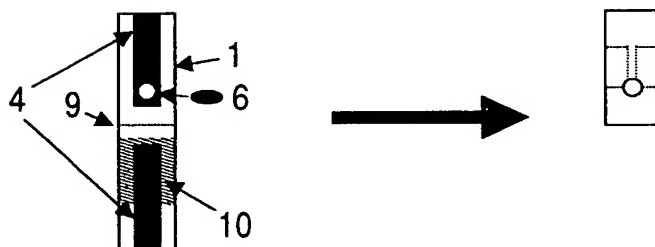

*FIG. 10*



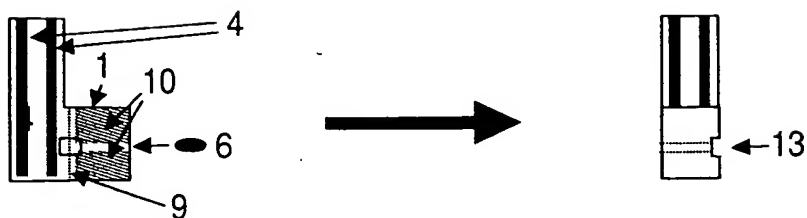



FIG. 11

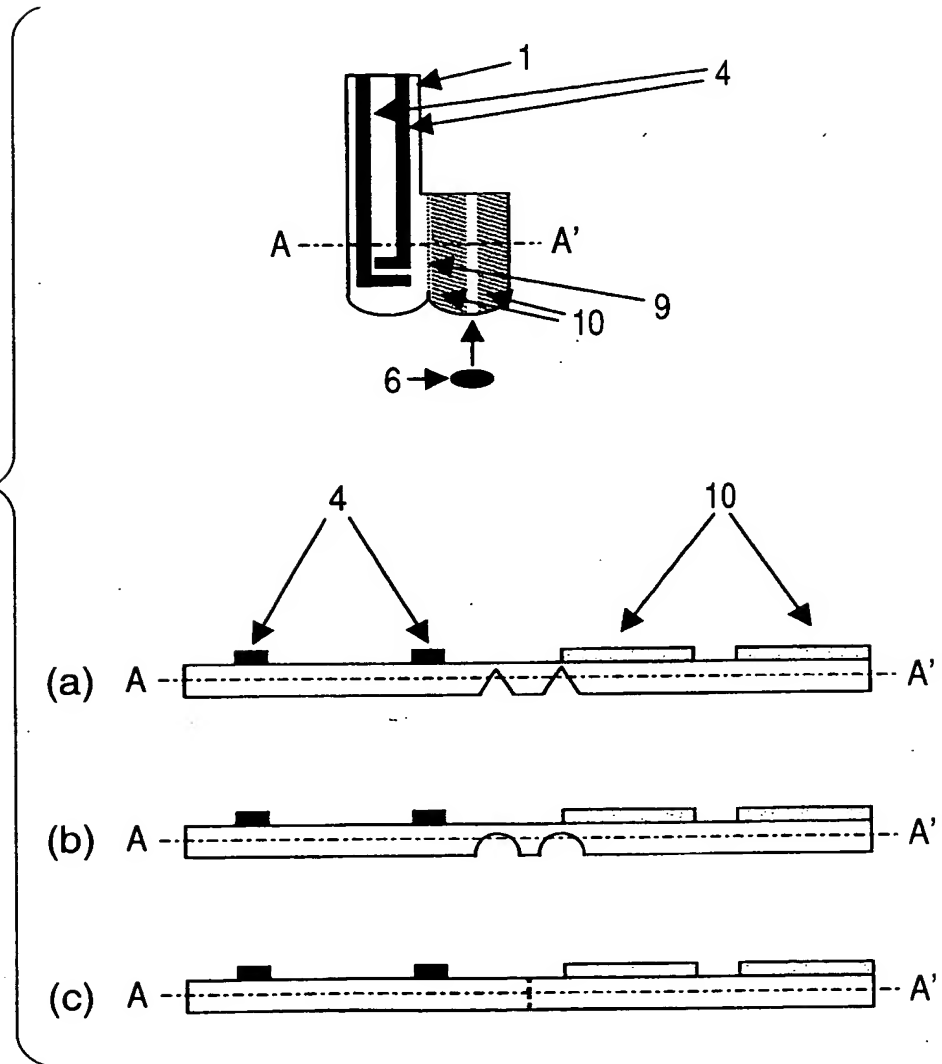


*FIG. 12*

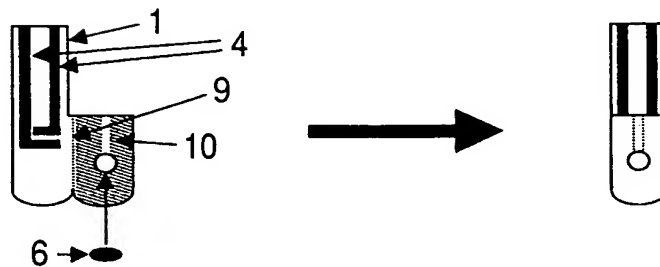


*FIG. 13*

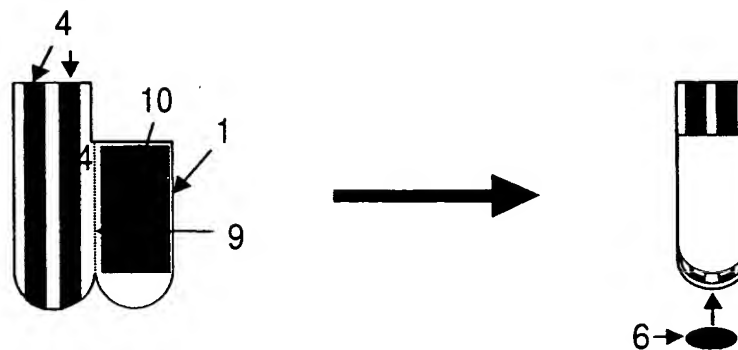


7/32

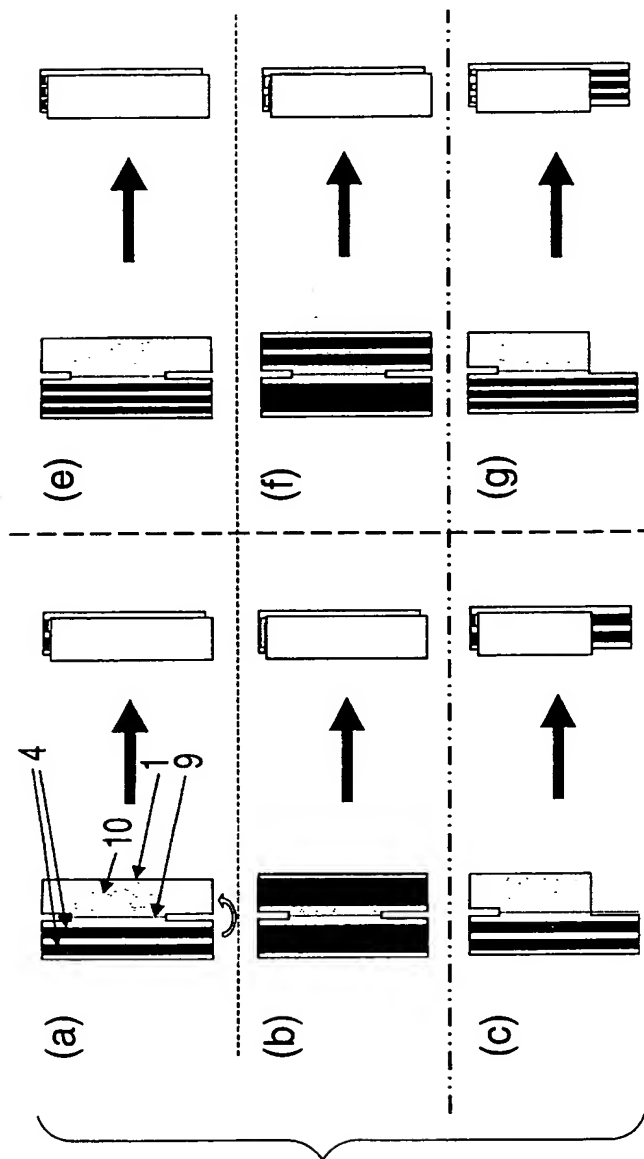


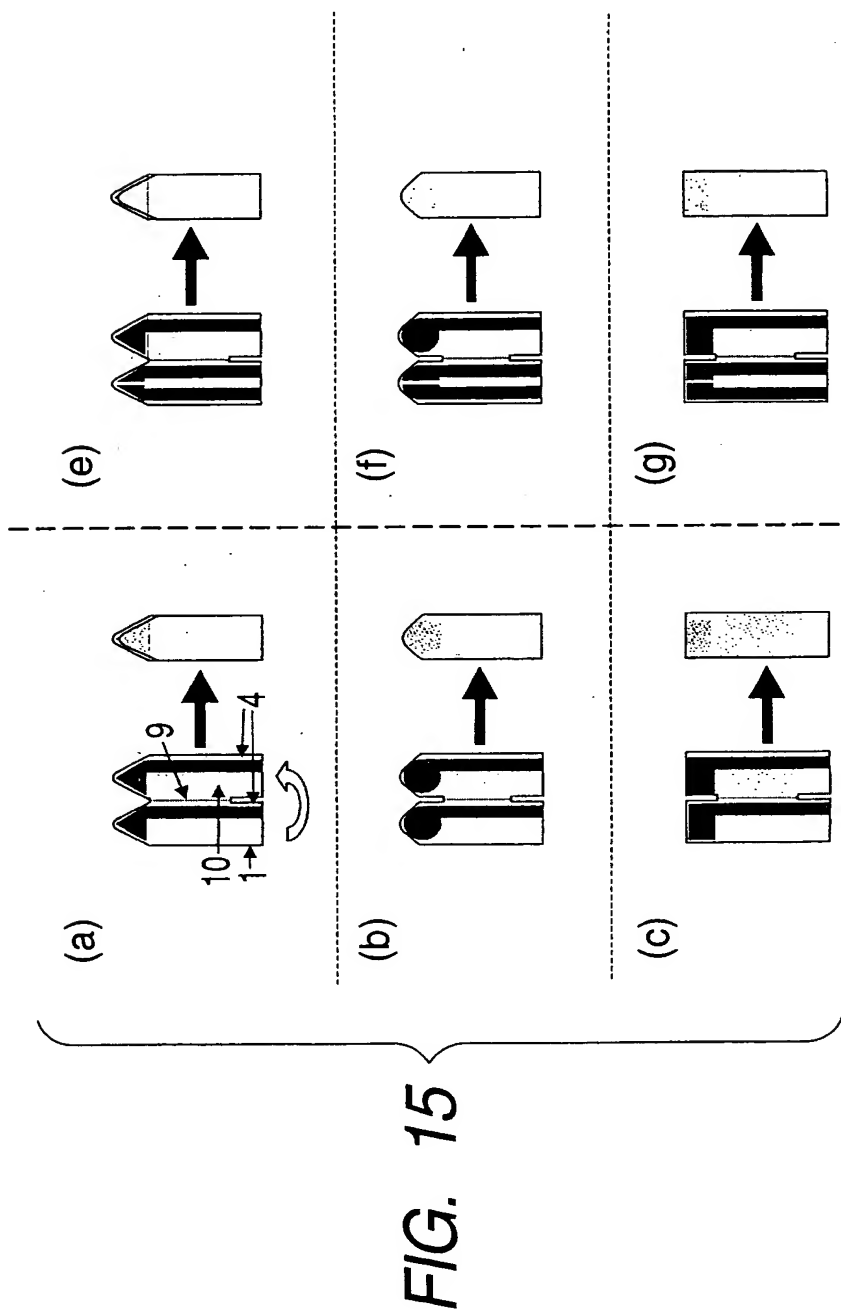



9 / 32

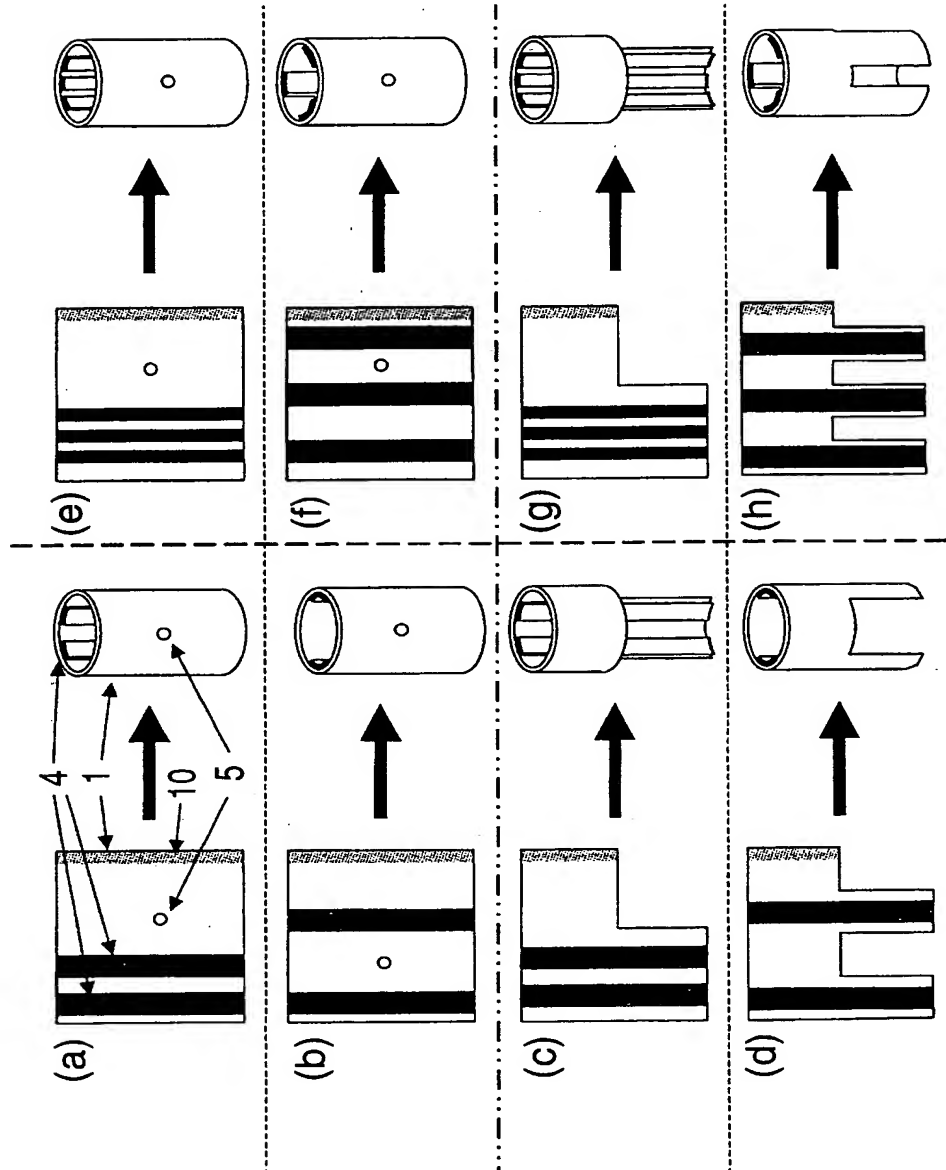

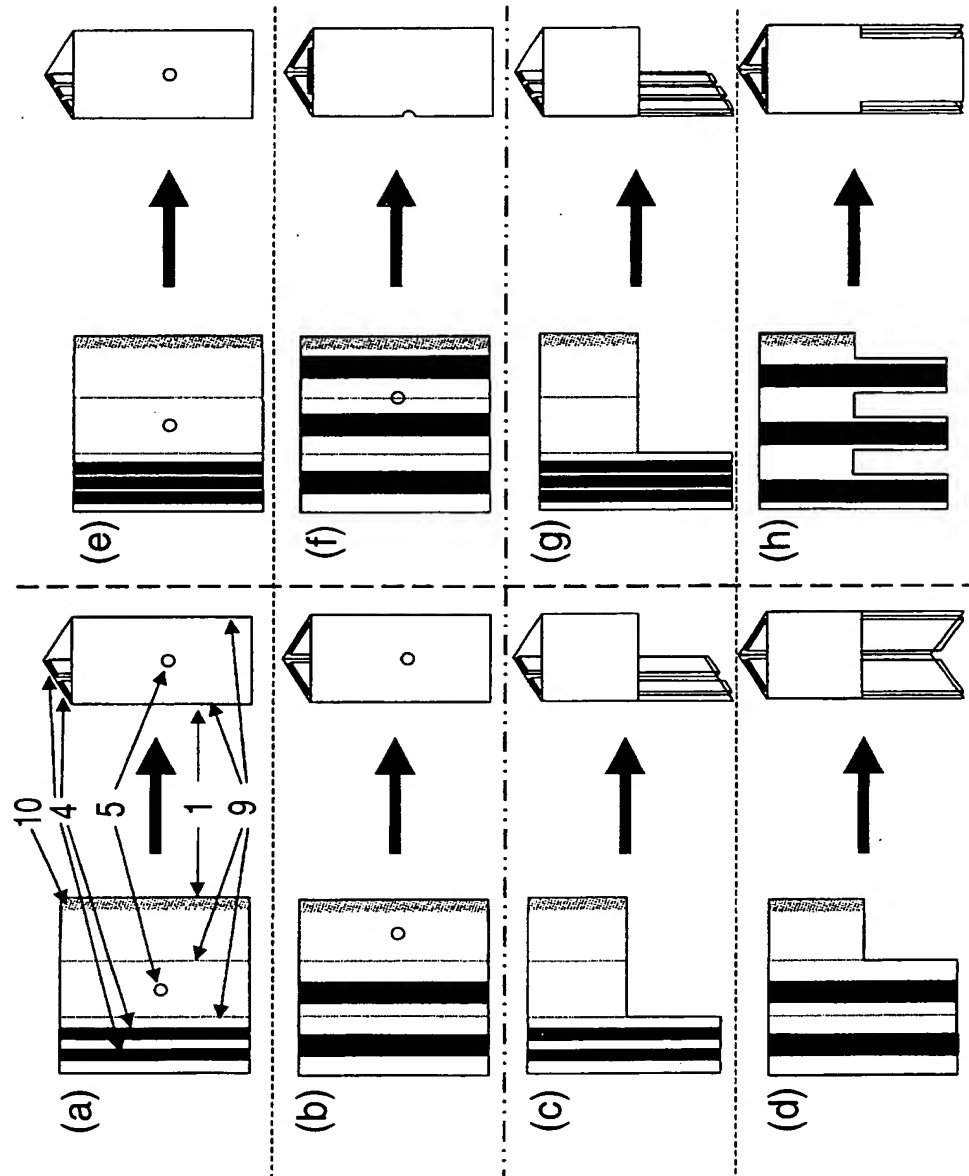

11 / 32



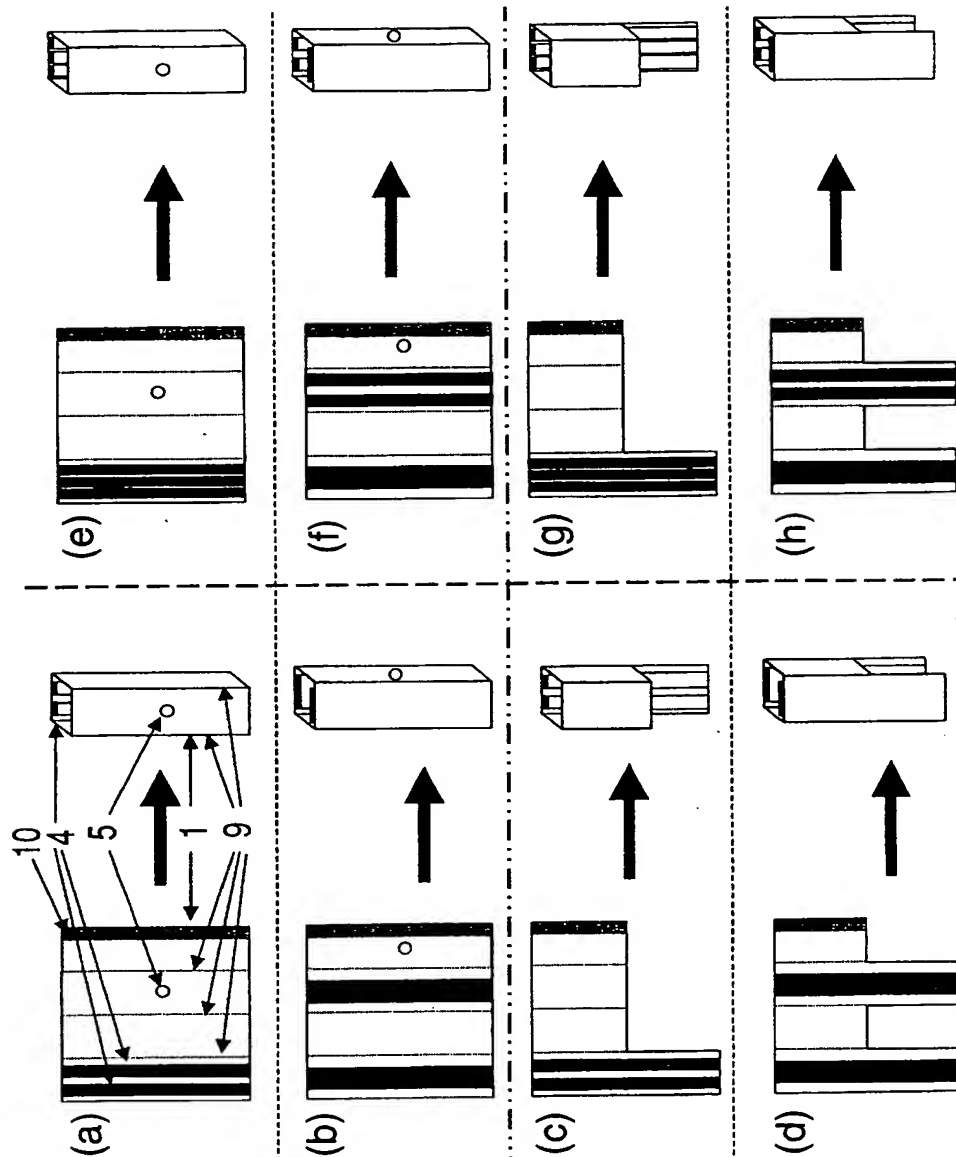



FIG. 18

*FIG. 19*

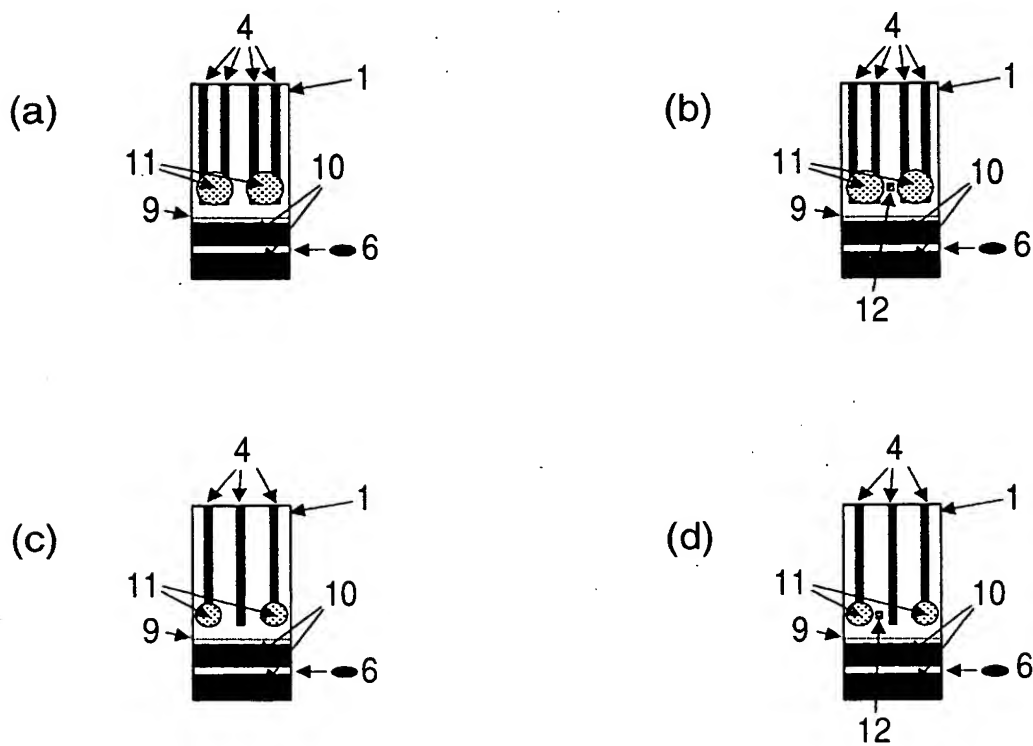


*FIG. 20*

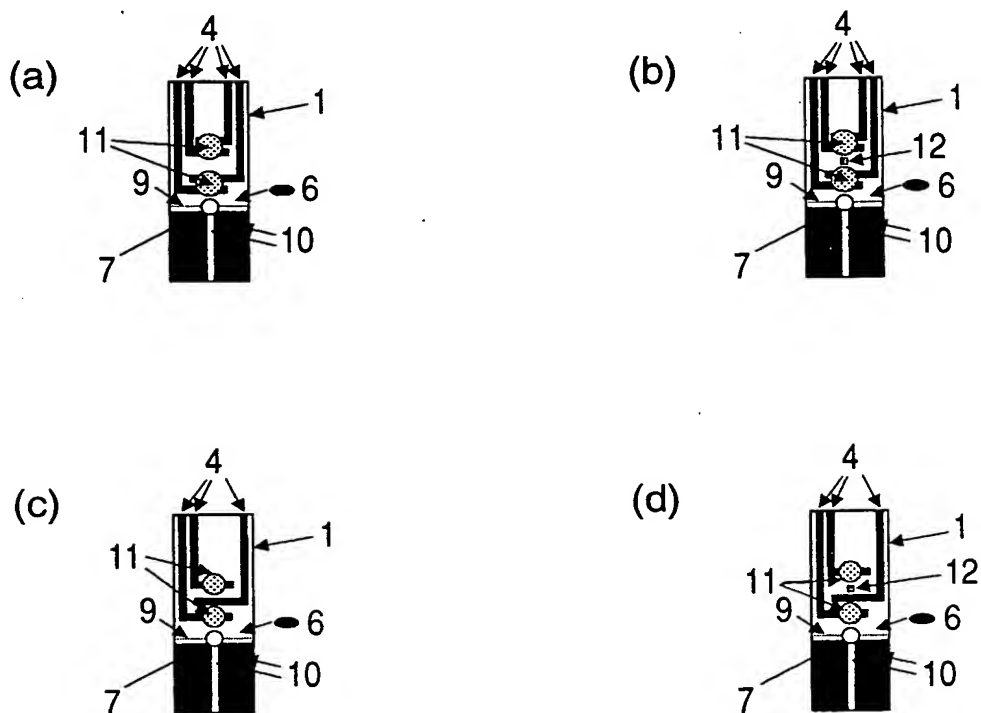

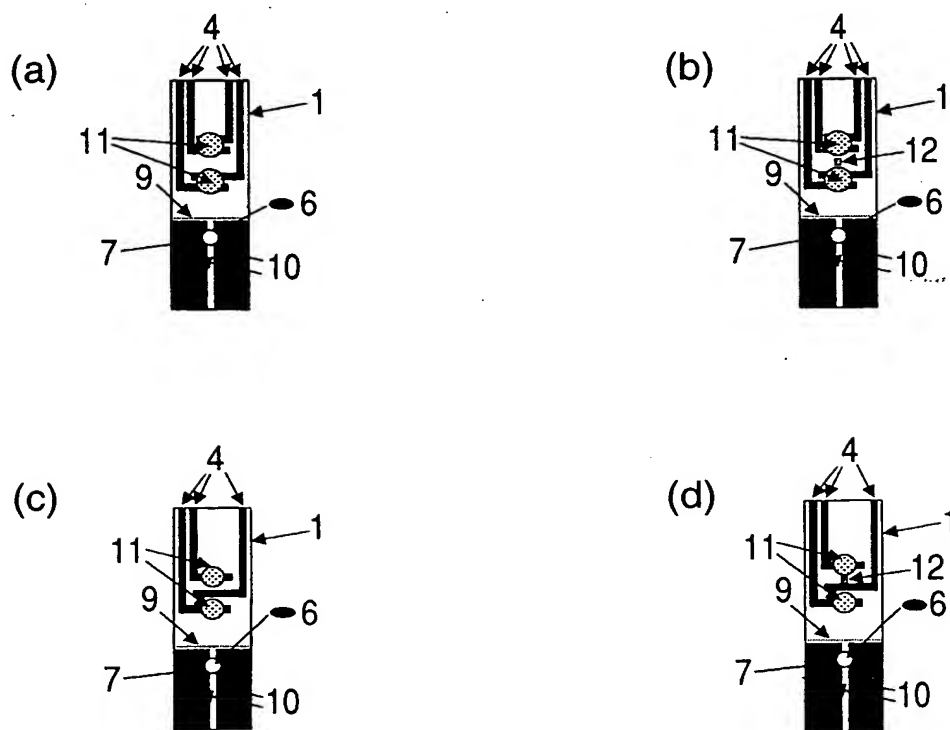*FIG. 21*


15 / 32

FIG. 22

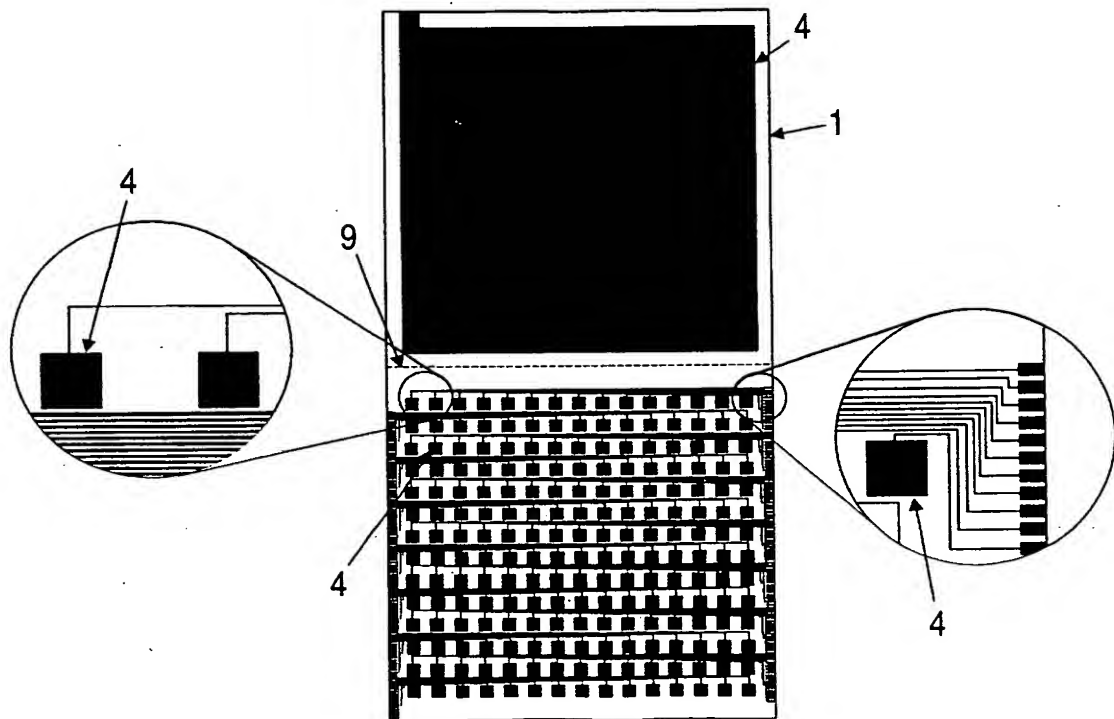


16 / 32


*FIG. 23*

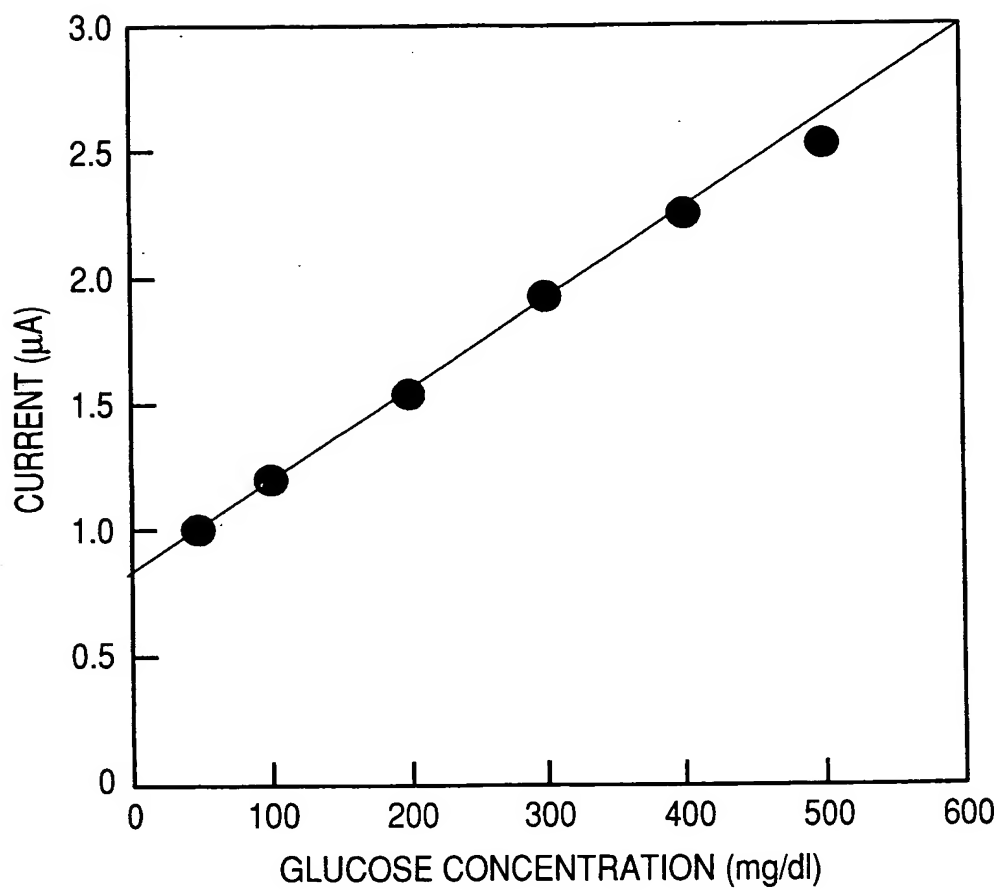




17 / 32

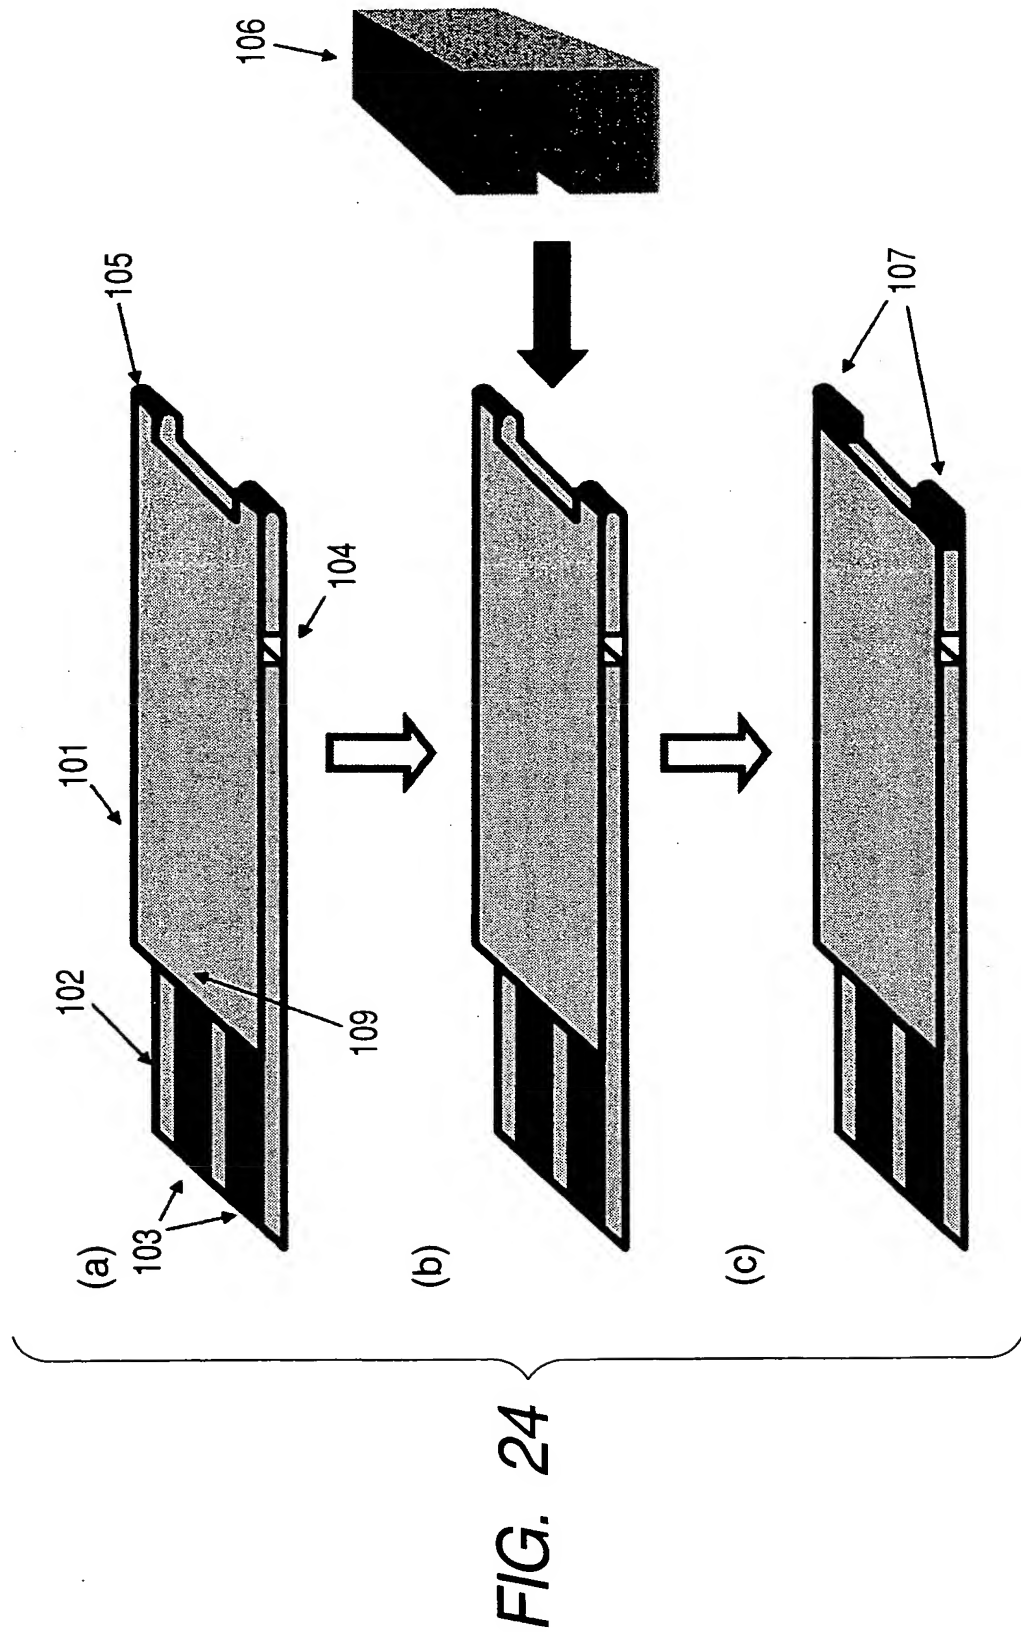

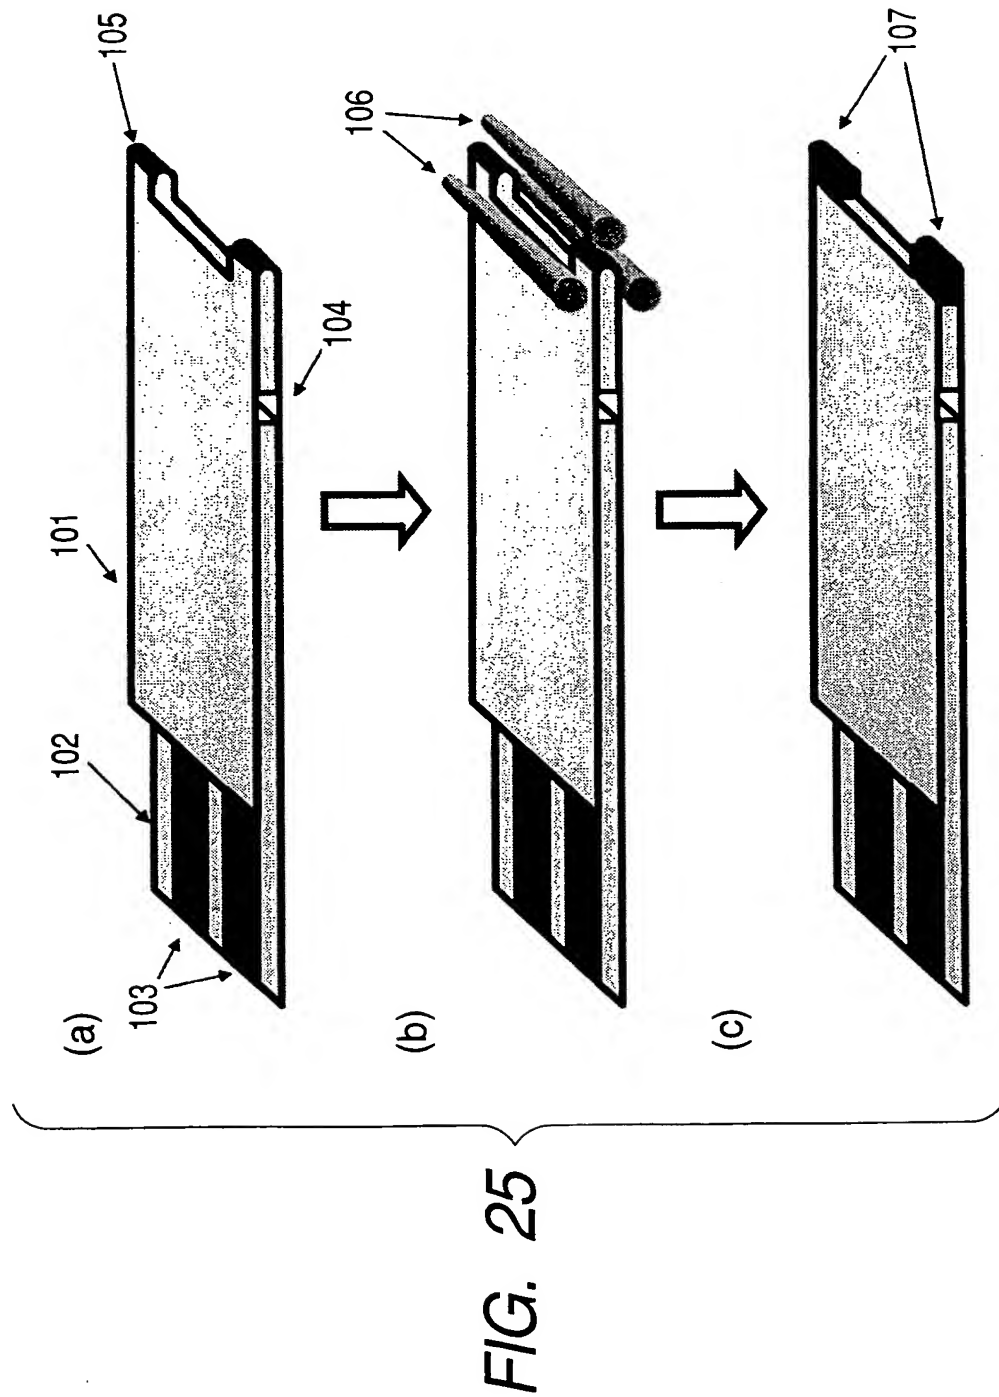

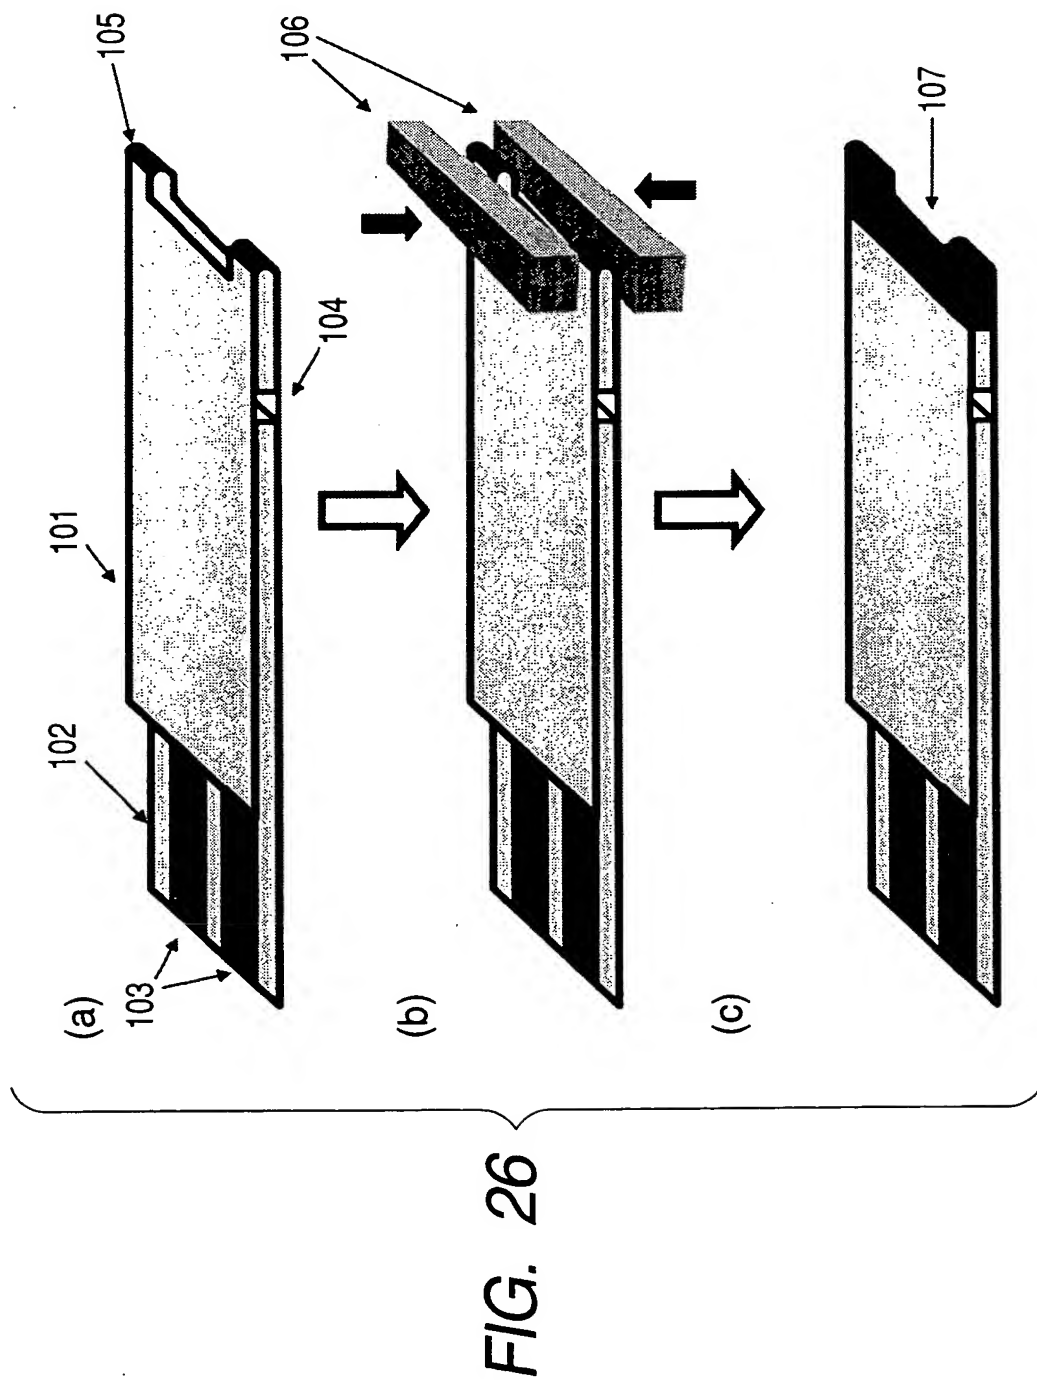

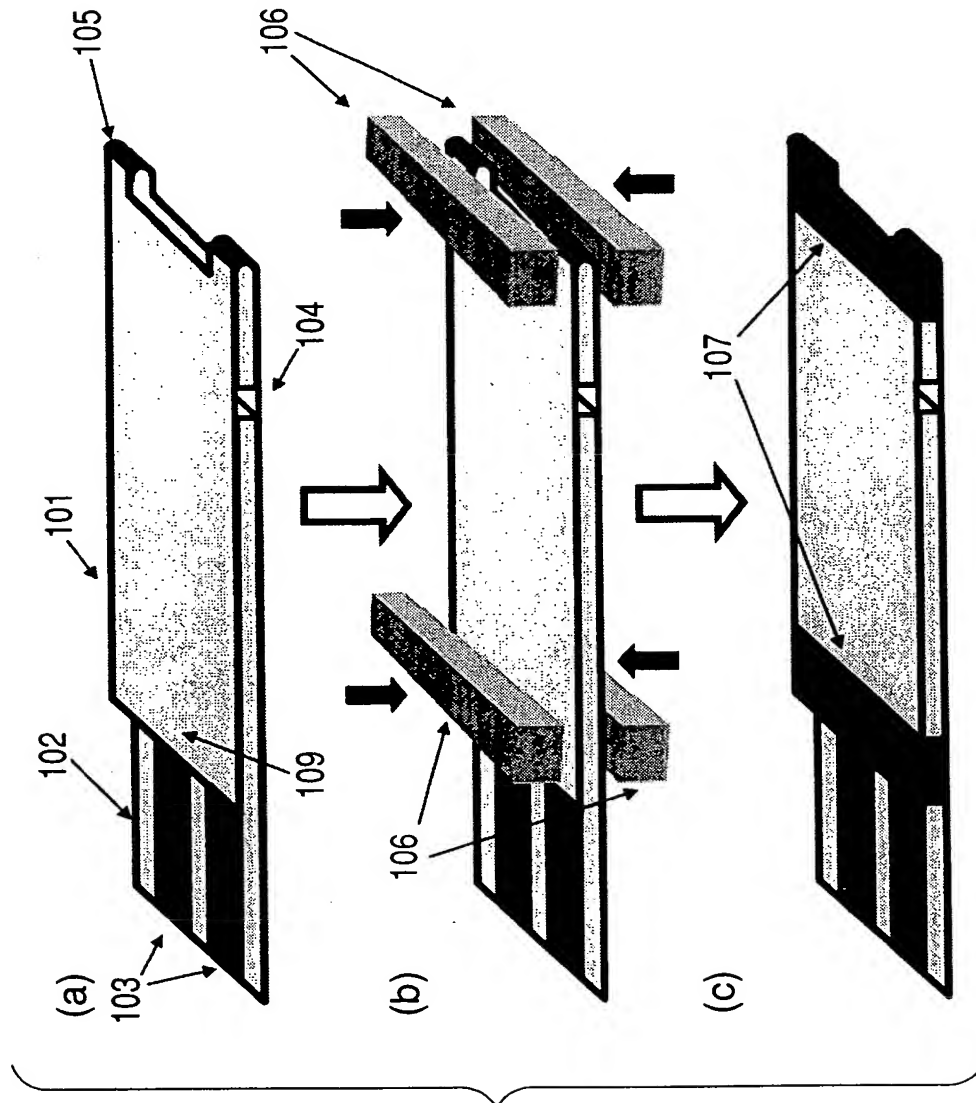


FIG. 27

21 / 32




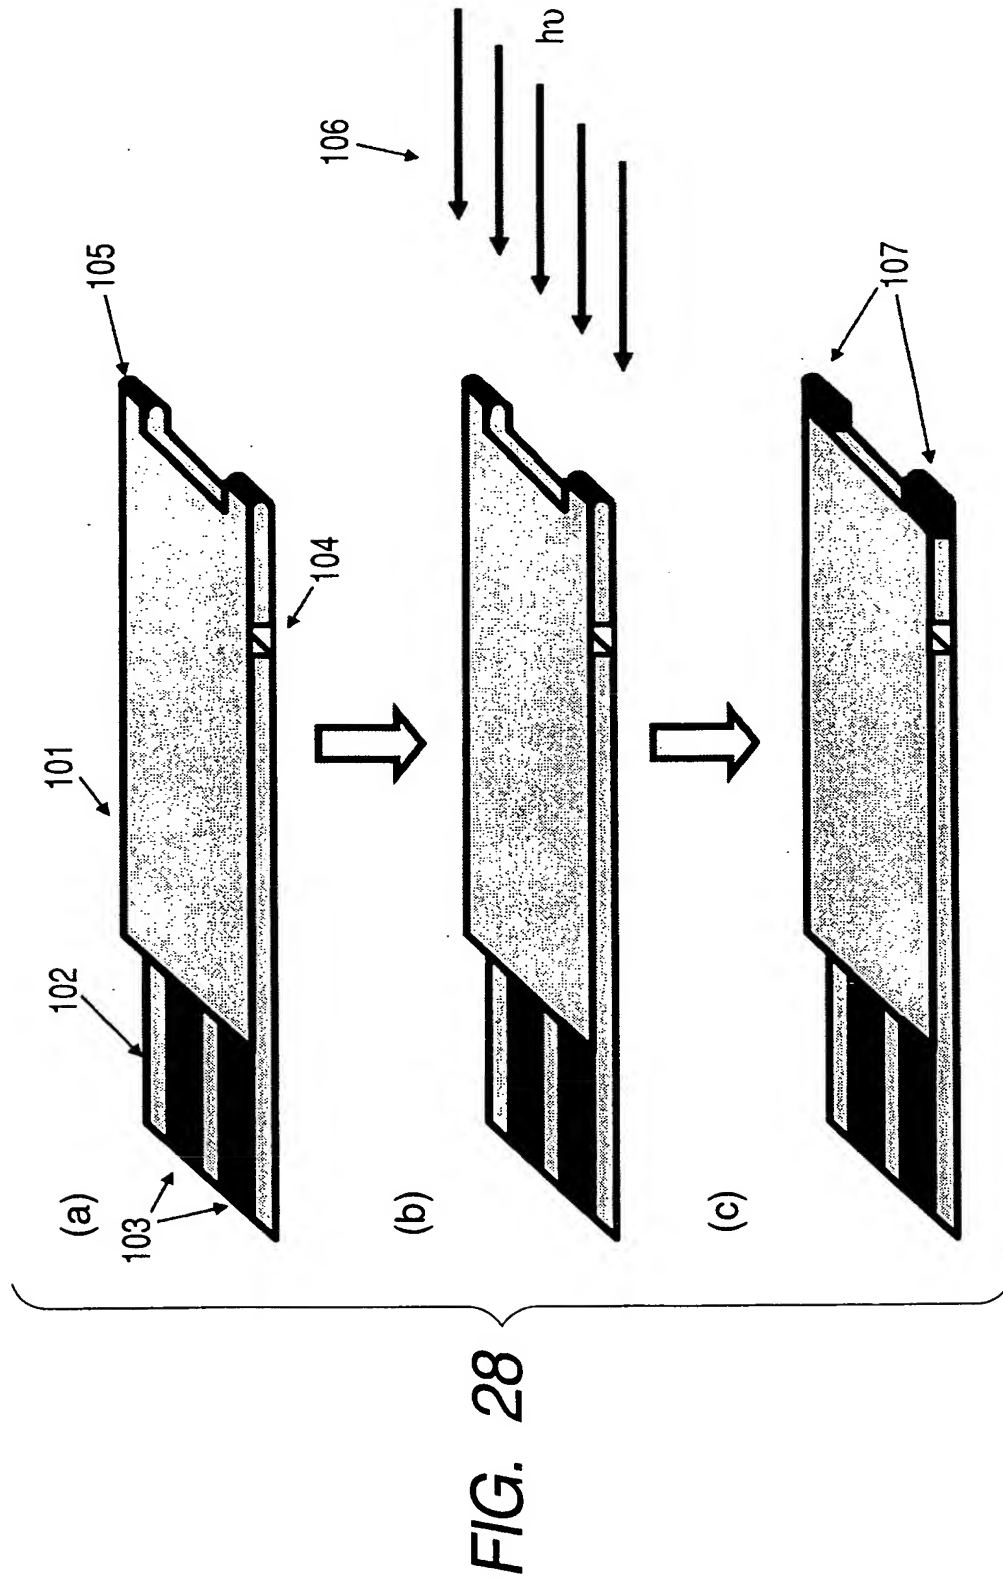


FIG. 29

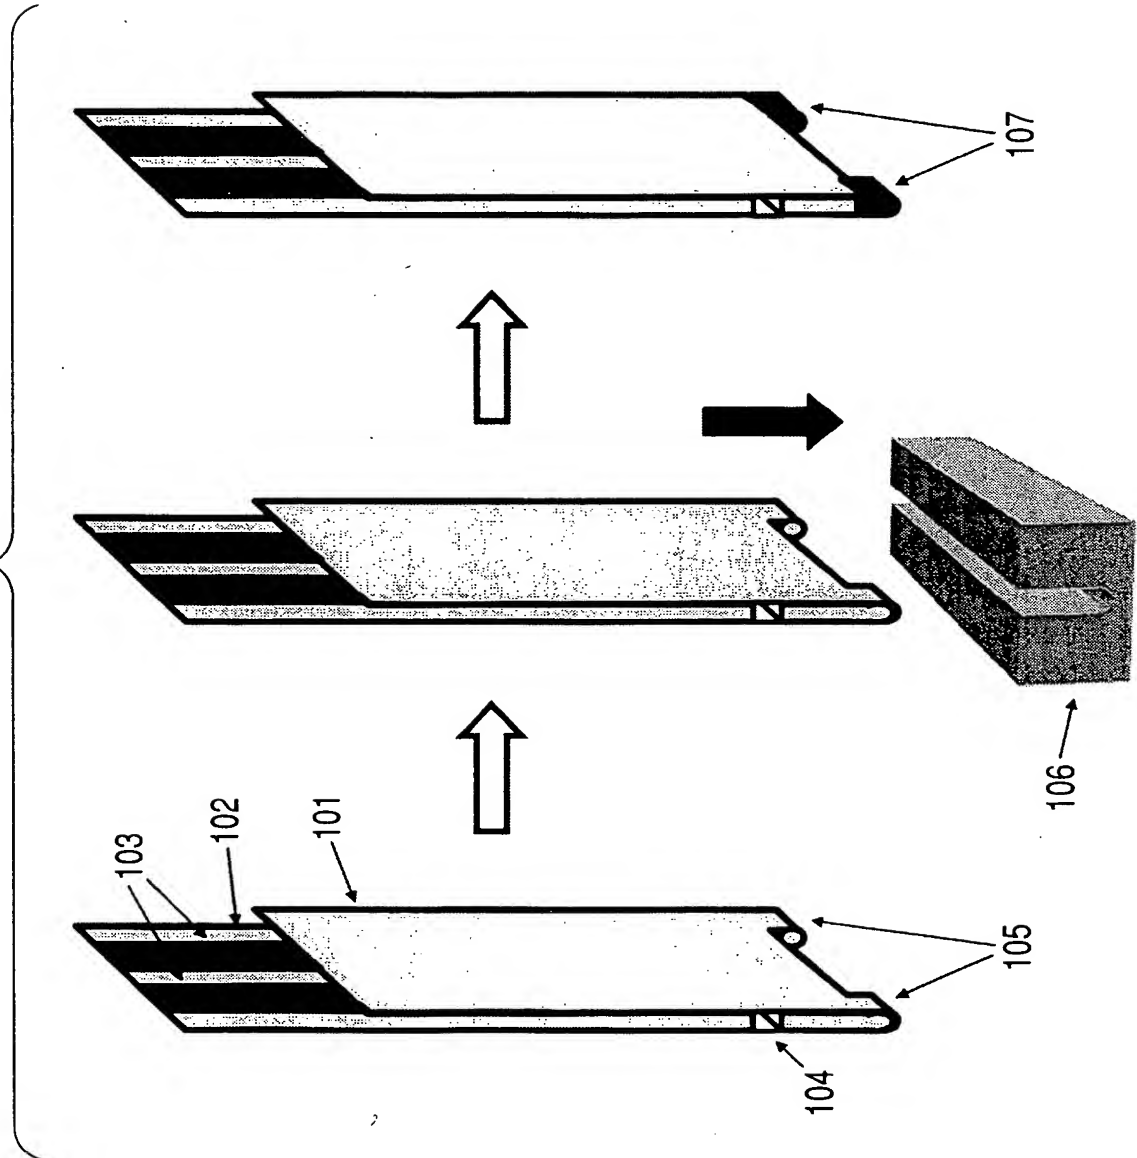


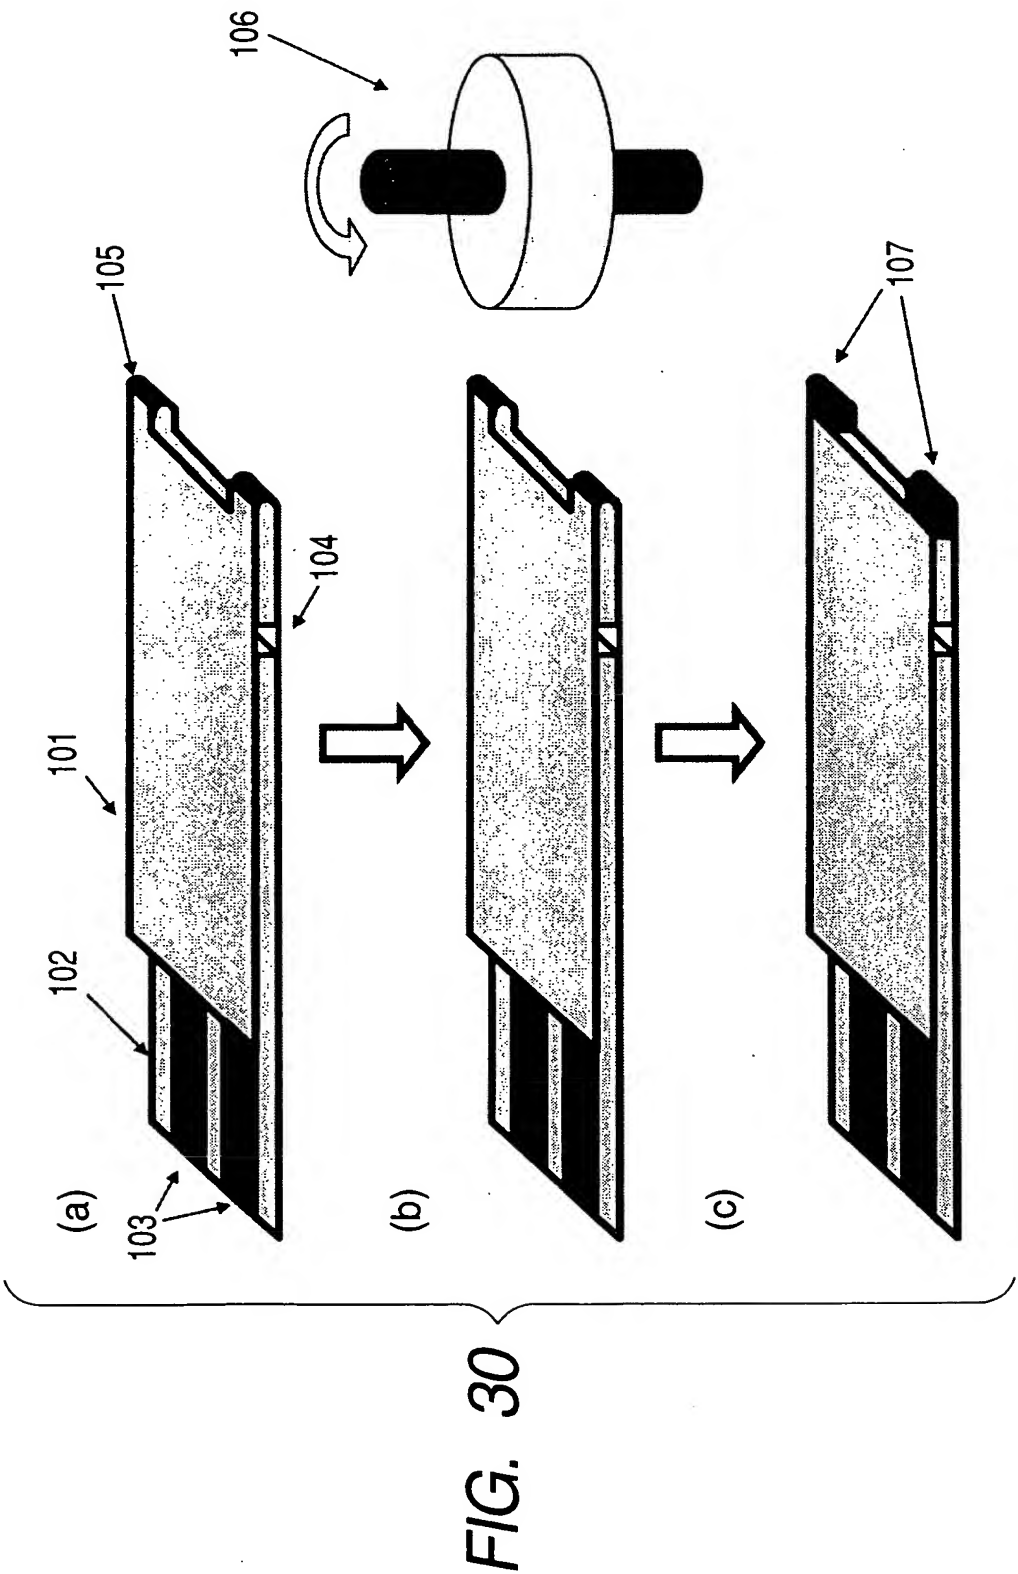


24 / 32

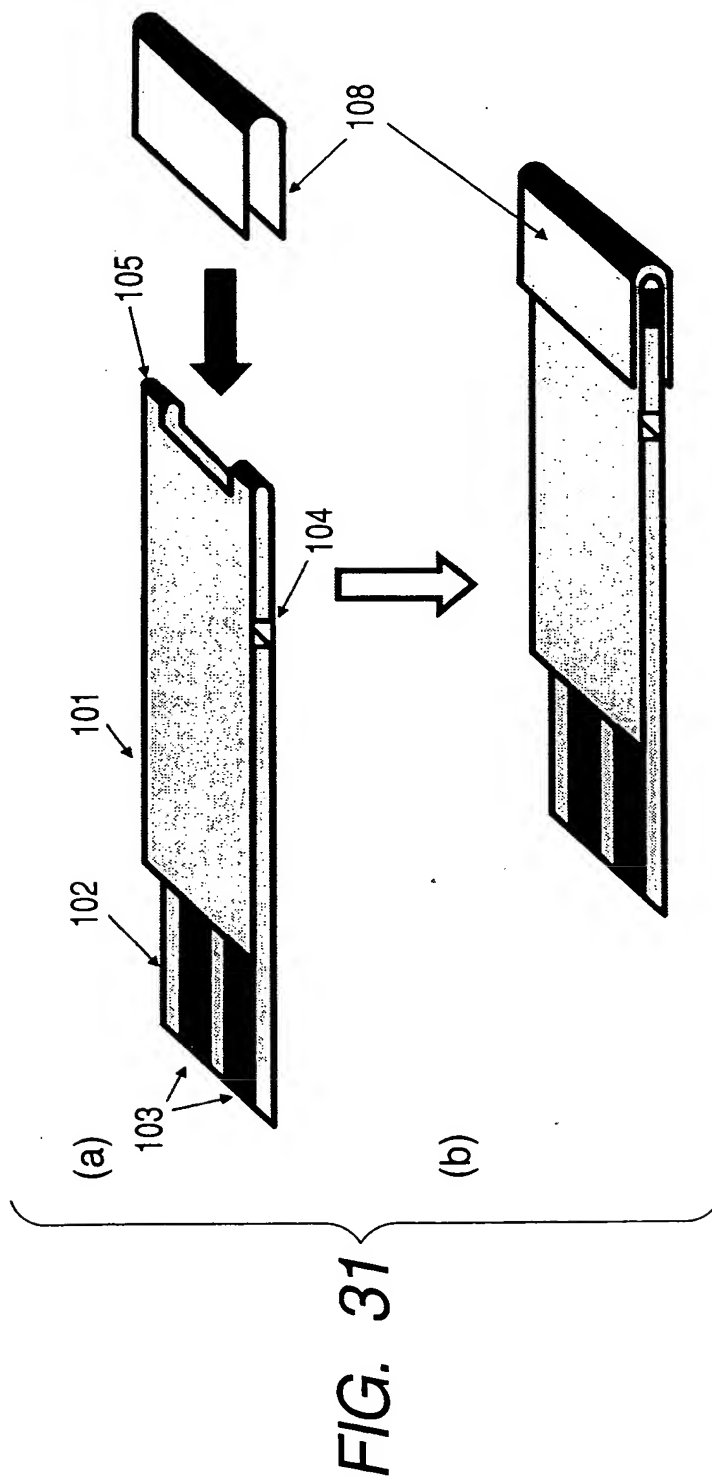




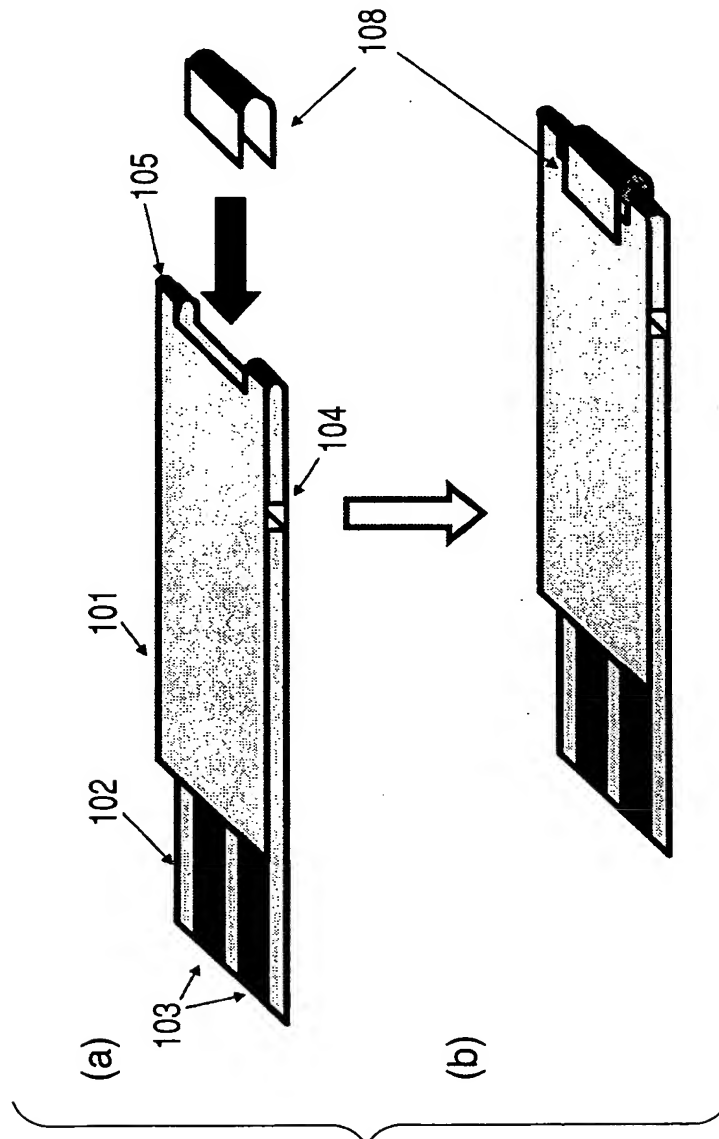

26 / 32

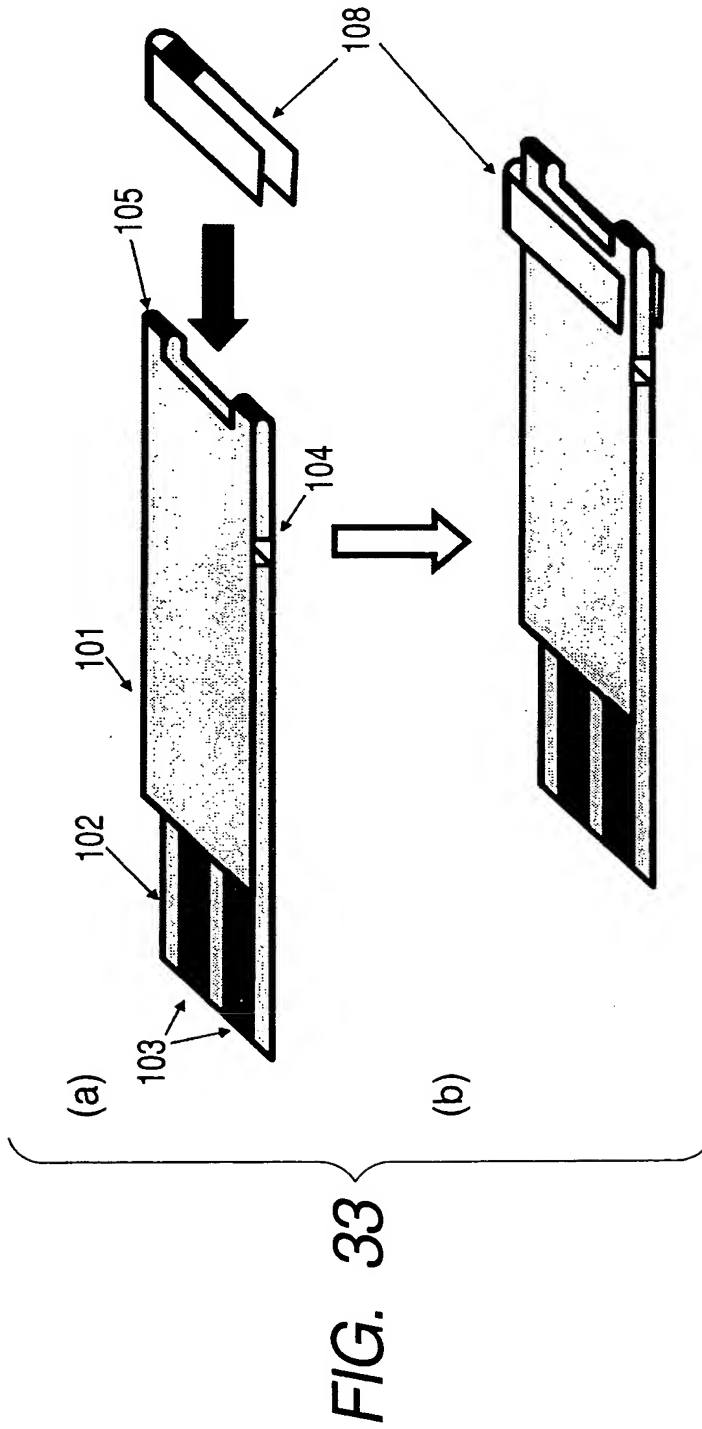

27 / 32

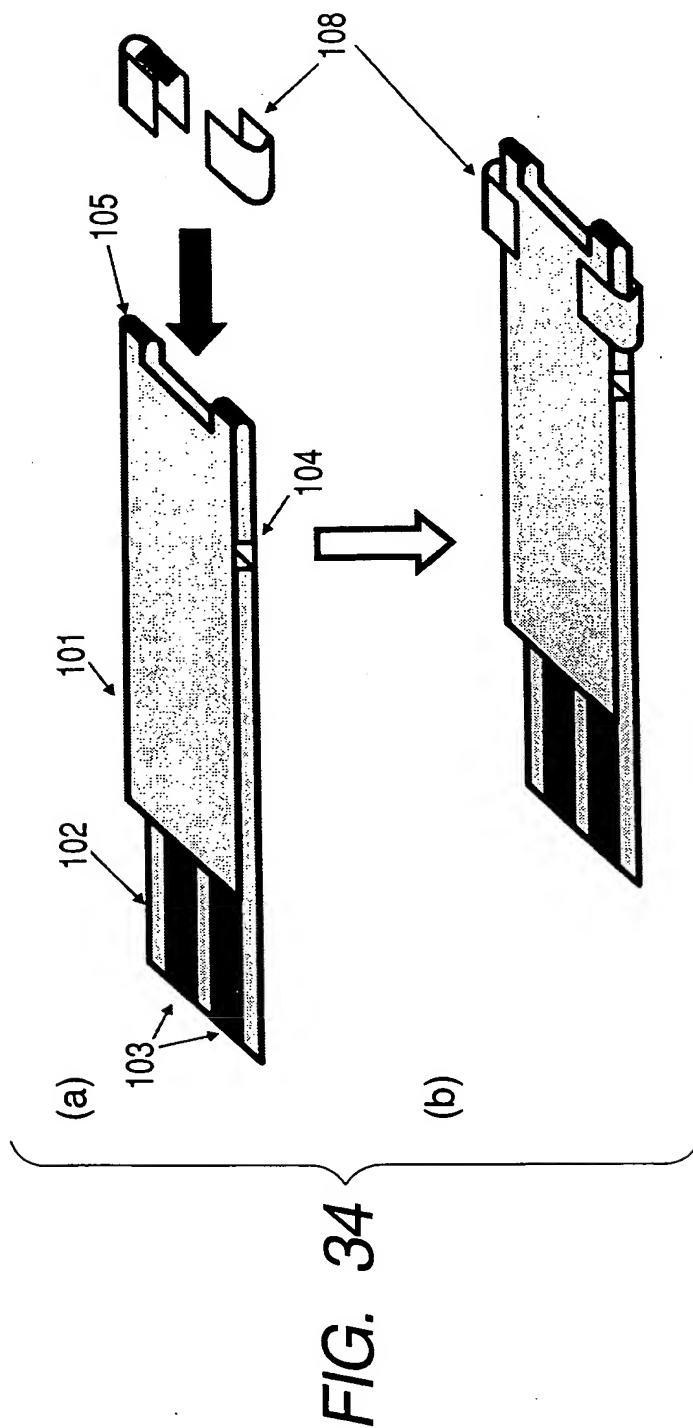



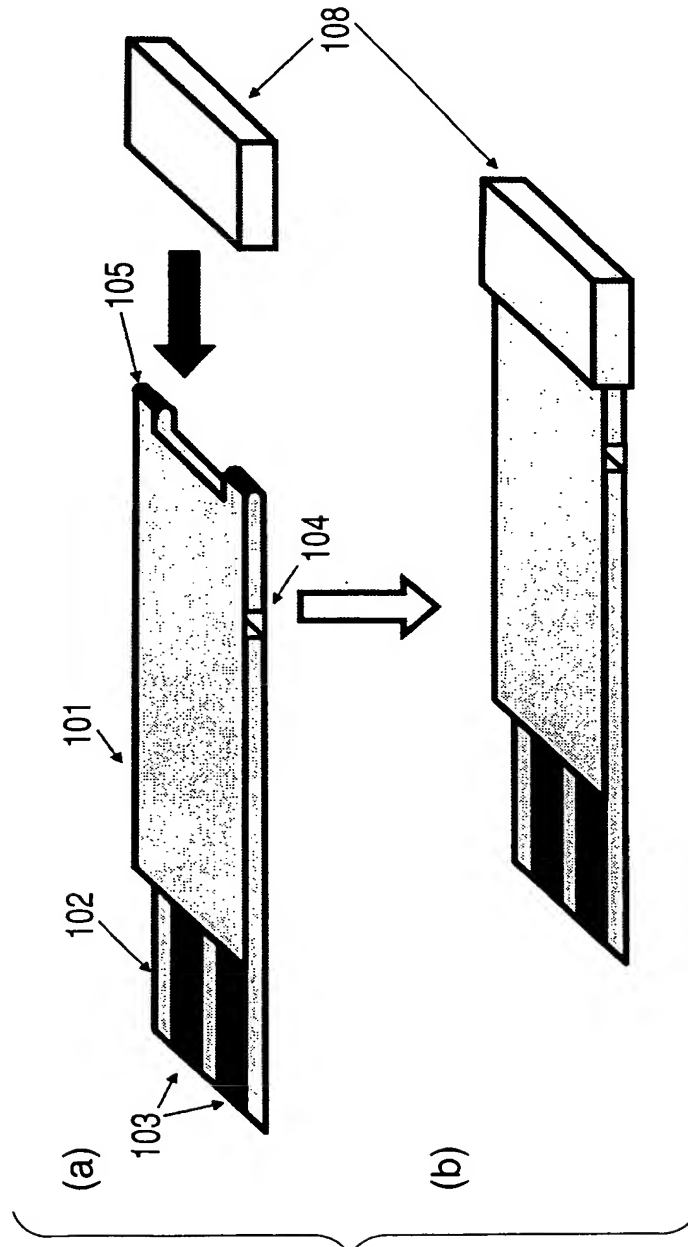


FIG. 35

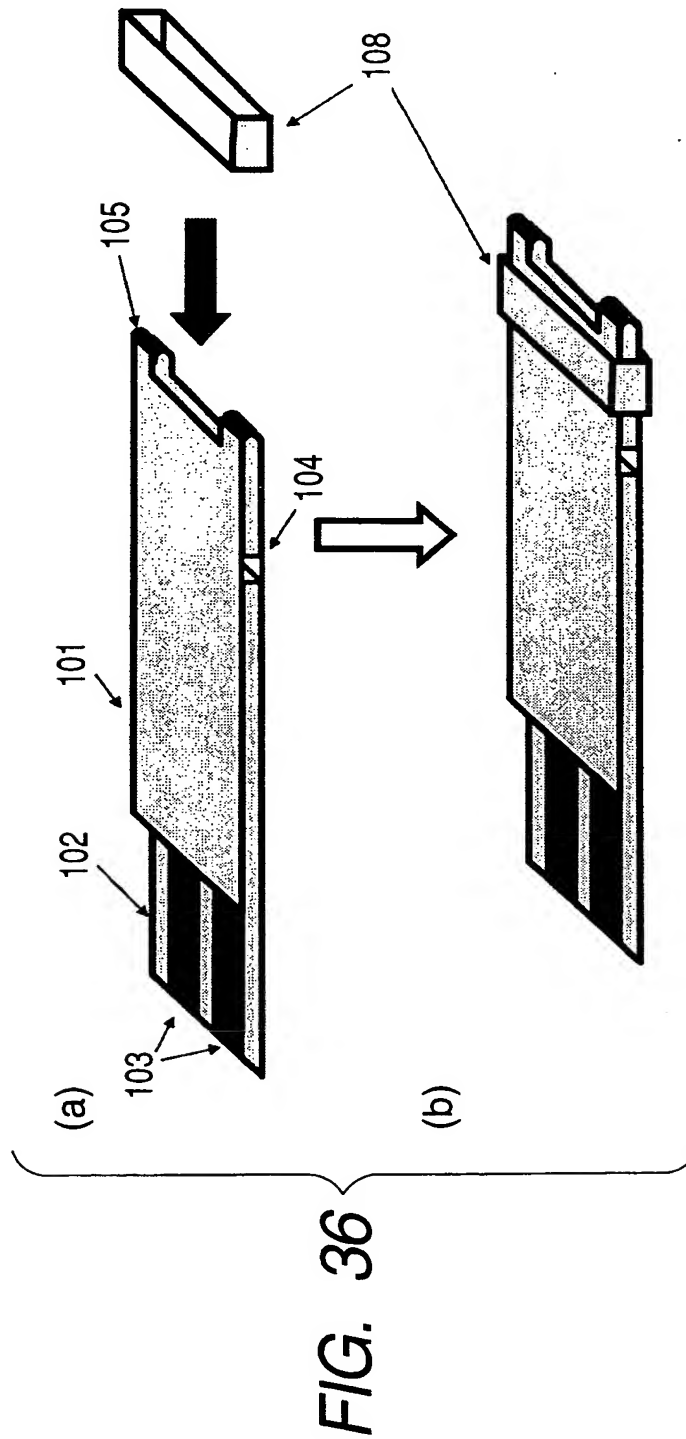

30 / 32

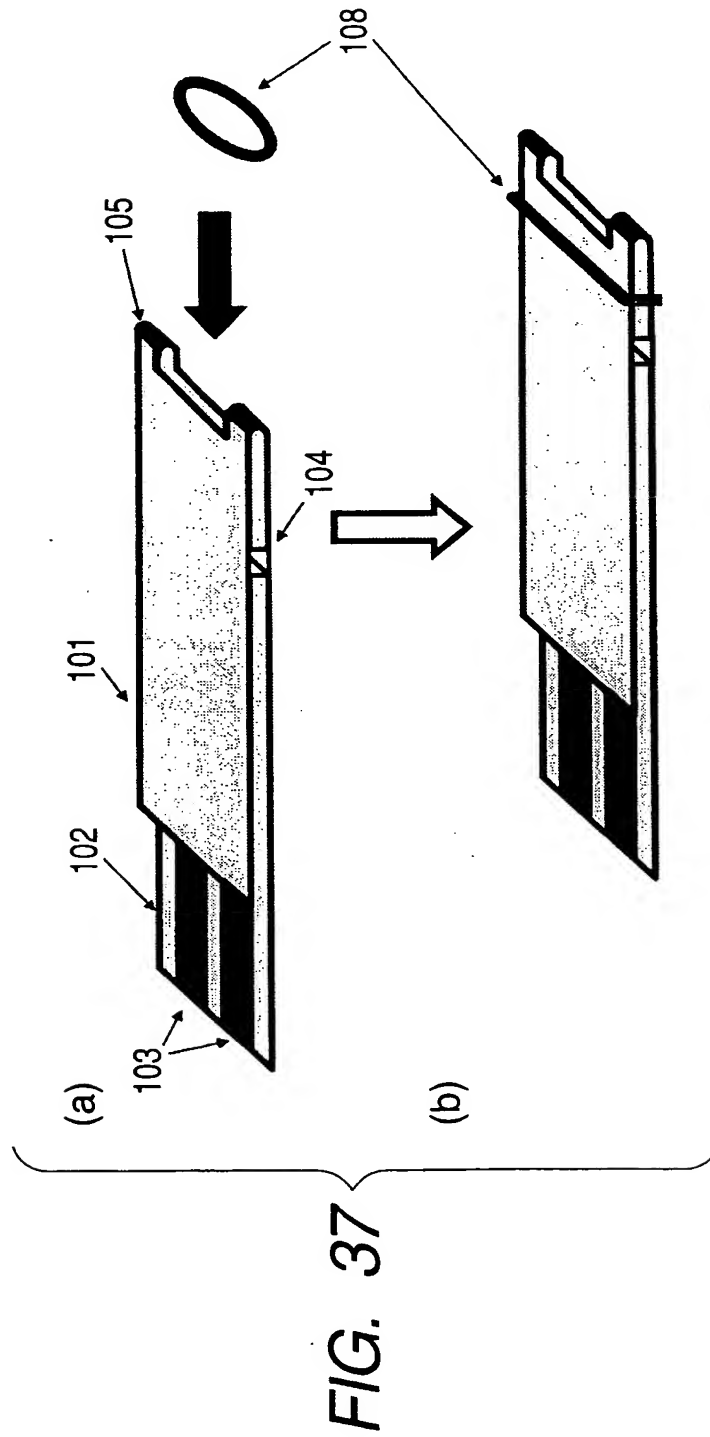

31 / 32

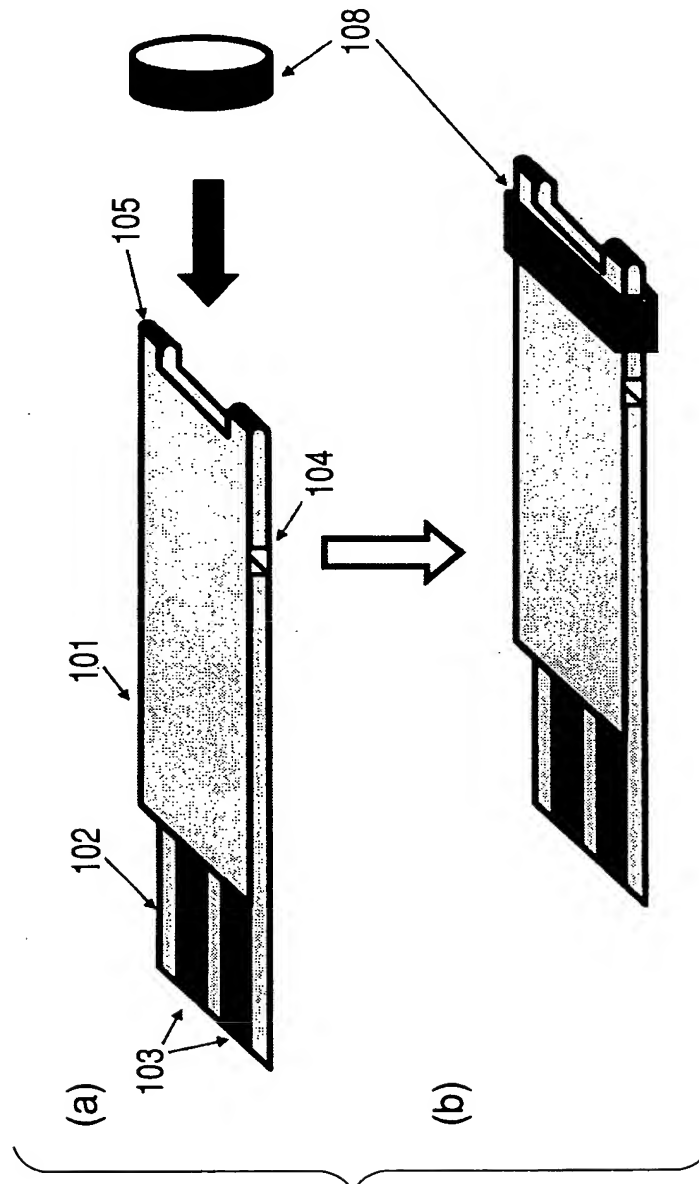


FIG. 38

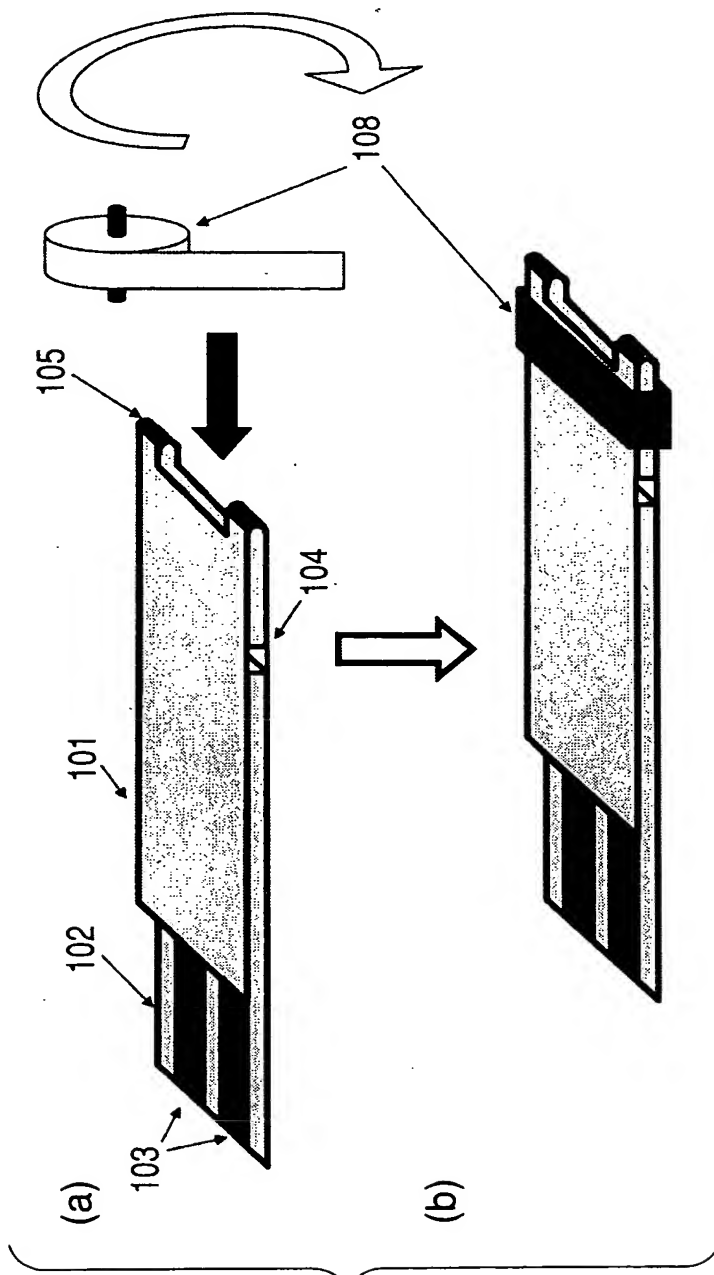


FIG. 39